

**FLUKE®**

# **Models 175, 177 & 179**

True RMS Multimeters

**Users Manual**

## **Table of Contents**

| Title                                                        | Page |
|--------------------------------------------------------------|------|
| Contacting Fluke.....                                        | 1    |
| "Warning" and "Caution" Statements .....                     | 1    |
| Unsafe Voltage .....                                         | 1    |
| Test Lead Alert .....                                        | 1    |
| Battery Saver ("Sleep Mode").....                            | 2    |
| Terminals .....                                              | 2    |
| Rotary Switch Positions.....                                 | 2    |
| Display .....                                                | 3    |
| MIN MAX AVG Recording Mode .....                             | 4    |
| Display HOLD and AutoHOLD Modes.....                         | 4    |
| YELLOW Button .....                                          | 4    |
| Display Backlight (Model 177 and 179 Only) .....             | 4    |
| Manual Ranging and Autoranging .....                         | 5    |
| Power-Up Options .....                                       | 5    |
| Making Basic Measurements .....                              | 6    |
| Measuring AC and DC Voltage .....                            | 6    |
| Measuring Resistance .....                                   | 6    |
| Measuring Capacitance.....                                   | 6    |
| Testing for Continuity.....                                  | 7    |
| Measuring Temperature (Model 179 Only) .....                 | 7    |
| Testing Diodes.....                                          | 7    |
| Measuring AC or DC Current .....                             | 8    |
| Understanding AC Zero Input Behavior of True RMS Meters..... | 8    |
| Measuring Frequency.....                                     | 9    |
| Using the Bar Graph .....                                    | 9    |
| Cleaning.....                                                | 10   |
| Testing the Fuses .....                                      | 10   |
| Replacing the Battery and Fuses .....                        | 10   |
| Specifications.....                                          | 11   |

**⚠ ⚠ Warning. Read before using the Meter:**

To avoid possible electrical shock or personal injury, follow these guidelines:

- ⇒ Use the Meter only as specified in this manual or the protection provided by the Meter might be impaired.
- ⇒ Do not use the Meter or test leads if they appear damaged, or if the Meter is not operating properly. If in doubt, have the Meter serviced.
- ⇒ Always use the proper terminals, switch position, and range for measurements.
- ⇒ Verify the Meter's operation by measuring a known voltage.
- ⇒ Do not apply more than the rated voltage, as marked on the Meter, between the terminals or between any terminal and earth ground.
- ⇒ Use caution with voltages above 30 V ac rms, 42 V ac peak, or 60 V dc. These voltages pose a shock hazard.
- ⇒ Replace the battery as soon as the low battery indicator (  ) appears.
- ⇒ Disconnect circuit power and discharge all high-voltage capacitors before testing resistance, continuity, diodes, or capacitance.
- ⇒ Do not use the Meter around explosive gas or vapor.
- ⇒ When using the test leads, keep your fingers behind the finger guards.
- ⇒ Remove test leads from the Meter before opening the Meter case or battery door.

**Symbols**


|                                                                                     |                                                                                        |                                                                                     |                                                                               |
|-------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------|-------------------------------------------------------------------------------|
|  | AC (Alternating Current)                                                               |  | Fuse                                                                          |
|  | DC (Direct Current)                                                                    |  | Conforms to European Union directives                                         |
|  | DC/AC                                                                                  |  | Canadian Standards Association                                                |
|  | Earth ground                                                                           |  | Double insulated                                                              |
|  | Important Information; see manual                                                      |  | Underwriters Laboratories, Inc.<br>Meter in accordance with IEC 61010-1. 54CJ |
|  | Battery (Low battery when shown on display.)                                           |  | Conforms to relevant Australian standards                                     |
|  | Inspected and licensed by TÜV<br>(Technischer Überwachungs Verein)<br>Product Services |  | VDE (Verband Deutscher Elektroniker)                                          |

**Models 175, 177 & 179**  
Users Manual

**Battery Saver ("Sleep Mode")**

The Meter enters the "Sleep mode" and blanks the display if there is no function change or button press for 20 minutes. To disable the Sleep mode, hold down the **YELLOW** button while turning the Meter on. The Sleep mode is always disabled in the MIN MAX AVG mode and the AutoHOLD mode.

**Terminals**

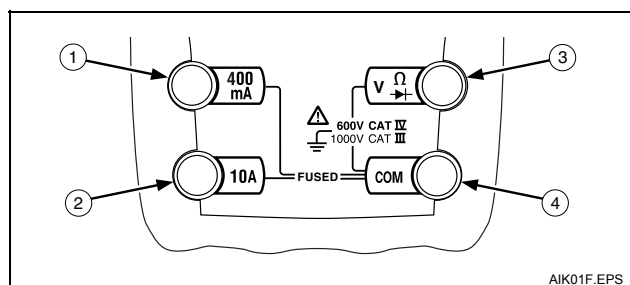


| Item | Description                                                                                                                       |
|------|-----------------------------------------------------------------------------------------------------------------------------------|
| 1    | Input terminal for AC and DC milliamp measurements to 400 mA and frequency measurements.                                          |
| 2    | Input terminal for AC and DC current measurements to 10 A and frequency measurements.                                             |
| 3    | Input terminal for voltage, continuity, resistance, diode, capacitance, frequency, and temperature (Model 179 only) measurements. |
| 4    | Common (return) terminal for all measurements.                                                                                    |

**Rotary Switch Positions**

| Switch Position         | Measurement Function                                                                                                                                     |
|-------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------|
| $\tilde{V}$<br>Hz       | AC voltage from 30.0 mV to 1000 V.<br>Frequency from 2 Hz to 99.99 kHz.                                                                                  |
| $\bar{V}$<br>Hz         | DC voltage 1 mV to 1000 V.<br>Frequency from 2 Hz to 99.99 kHz.                                                                                          |
| mV<br>⌚                 | DC mV 0.1 mV to 600 mV.<br>Temperature – 40 °C to + 400 °C<br>– 40 °F to + 752 °F                                                                        |
| Ω<br>⌚                  | Ohms from 0.1 Ω to 50 MΩ.<br>Farads from 1 nF to 9999 μF.                                                                                                |
| ⌚<br>⌚                  | Beeper turns on at <25 Ω and turns off at >250 Ω.<br>Diode test. Displays OL above 2.4 V.                                                                |
| $\tilde{mA}$<br>Hz      | AC mA from 3.00 mA to 400 mA<br>DC mA from 0.01 mA to 400 mA<br>Frequency of AC mA 2 Hz to 30 kHz.                                                       |
| $\tilde{A}$<br>~A<br>Hz | AC A from 0.300 A to 10 A<br>DC A from 0.001 A to 10 A<br>>10.00 display flashes.<br>>20 A, <b>OL</b> is displayed.<br>Frequency of AC A 2 Hz to 30 kHz. |

Note: AC voltage and current AC-coupled, true RMS, up to 1 kHz.

## Display

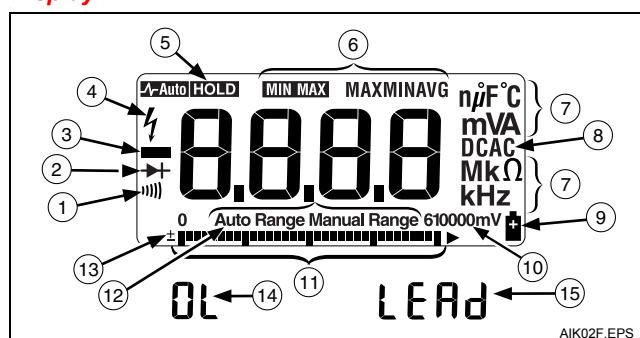

| No. | Symbol                                 | Meaning                                                                                                                                                                                                                                                         |
|-----|----------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1   |                                        | Continuity test.                                                                                                                                                                                                                                                |
| 2   |                                        | Diode test.                                                                                                                                                                                                                                                     |
| 3   |                                        | Negative readings.                                                                                                                                                                                                                                              |
| 4   |                                        | Unsafe voltage. Voltage $\geq 30$ V, or voltage overload (OL)                                                                                                                                                                                                   |
| 5   | <b>HOLD</b><br>                        | Display HOLD is enabled. Display freezes present reading.<br>In MIN MAX AVG mode, MIN MAX AVG recording is interrupted.<br>AutoHOLD is enabled. Display holds present reading until it detects new stable input. Then the Meter beeps and displays new reading. |
| 6   | <b>MIN MAX</b><br><b>MAX, MIN, AVG</b> | MIN MAX AVG enabled.<br>Maximum, minimum, average or present reading.                                                                                                                                                                                           |

| No. | Symbol                                   | Meaning                                                                                                   |
|-----|------------------------------------------|-----------------------------------------------------------------------------------------------------------|
| 7   | nF, F, °F, °C<br>mVA, MΩ, kHz            | Measurement units.                                                                                        |
| 8   | DC, AC                                   | Direct current, alternating current.                                                                      |
| 9   |                                          | Low battery. Replace battery.                                                                             |
| 10  | 610000mV                                 | All possible ranges.                                                                                      |
| 11  | Bar graph                                | Analog display.                                                                                           |
| 12  | <b>Auto Range</b><br><b>Manual Range</b> | The Meter selects the range with the best resolution.<br>The user selects the range.                      |
| 13  | $\pm$                                    | Bar graph polarity.                                                                                       |
| 14  | OL                                       | The input out of range.                                                                                   |
| 15  | LEAd                                     | Test lead alert. Displayed when the rotary switch is moved <u>to</u> or <u>from</u> the mA or A position. |

| Error Messages  |                                                                                                   |
|-----------------|---------------------------------------------------------------------------------------------------|
| <b>bAtt</b>     | Replace the battery immediately.                                                                  |
| <b>diSC</b>     | In the capacitance function, too much electrical charge is present on the capacitor being tested. |
| <b>EEPr Err</b> | Invalid EEPROM data. Have Meter serviced.                                                         |
| <b>CAL Err</b>  | Invalid calibration data. Calibrate Meter.                                                        |
| <b>OPEn</b>     | Open thermocouple is detected.                                                                    |

### **MIN MAX AVG Recording Mode**

The MIN MAX AVG recording mode captures the minimum and maximum input values, and calculates a running average of all readings. When a new high or low is detected, the Meter beeps.

#### *Note*

*For DC functions, accuracy is the specified accuracy of the measurement function  $\pm 12$  counts for changes longer than 350 ms in duration.*

*For AC functions, accuracy is the specified accuracy of the measurement function  $\pm 40$  counts for changes longer than 900 ms in duration.*

To use MIN MAX AVG recording:

- ⇒ Make sure that the Meter is in the desired measurement function and range. (Autoranging is disabled in the MIN MAX AVG mode.)
- ⇒ Press **MIN MAX** to activate MIN MAX AVG mode. **MIN MAX** and **MAX** light, and the highest reading detected since entering MIN MAX AVG is displayed.
- ⇒ Press **MIN MAX** to step through the low (**MIN**), average (**AVG**), and present readings.
- ⇒ To pause MIN MAX AVG recording without erasing stored values, press **HOLD**. **HOLD** is displayed.  
To resume MIN MAX AVG recording, press **HOLD** again. **HOLD** turns off.
- ⇒ To exit and erase stored readings, press MIN MAX for 1 second or turn the rotary switch.

### **Display HOLD and AutoHOLD Modes**

#### **⚠ ⚠ Warning**

**To avoid electric shock, do not use the Display HOLD or AutoHOLD mode to determine if a circuit is live. Unstable or noisy readings will not be captured.**

In the Display HOLD mode, the Meter holds the reading on the display.

In the AutoHOLD mode, the Meter holds the reading on the display until it detects a new stable reading. Then the Meter beeps and displays the new reading.

- ⇒ Press **HOLD** to activate Display HOLD. **HOLD** lights.
- ⇒ Press **HOLD** again to activate AutoHOLD. **AutoHOLD** lights.
- ⇒ Press **HOLD** again to resume normal operation.

To resume normal operation at any time, press **HOLD** for 1 second or turn the rotary switch.

### **YELLOW Button**

Press the **YELLOW** button to select alternate measurement functions on a rotary switch setting, e.g., to select DC mA, DC A, Hz, temperature (Model 179 only), capacitance, diode test.

### **Display Backlight (Model 177 and 179 Only)**

Press  to toggle the backlight on and off. The backlight automatically turns off after 2 minutes.

### Manual Ranging and Autoranging

The Meter has both Manual range and Autorange modes.

- ⇒ In the Autorange mode, the Meter selects the range with the best resolution.
- ⇒ In the Manual Range mode, you override Autorange and select the range yourself.

When you turn the Meter on, it defaults to Autorange and **Auto Range** is displayed.

1. To enter the Manual Range mode, press **RANGE**.  
**Manual Range** is displayed.
2. In the Manual Range mode, press **RANGE** to increment the range. After the highest range, the Meter wraps to the lowest range.

*Note*

*You cannot manually change the range in the MIN MAX AVG, or Display HOLD modes.*

*If you press **RANGE** while in MIN MAX AVG, or Display HOLD, the Meter beeps twice, indicating an invalid operation, and the range does not change.*

3. To exit Manual Range, press **RANGE** for 1 second or turn the rotary switch.  
The Meter returns to Autorange and **Auto Range** is displayed.

### Power-Up Options

To select a Power-Up Option, hold down the button indicated while turning the Meter from OFF to any switch position.

Power-Up Options are cancelled when the Meter is turned OFF.

| Button                                                                                          | Power-Up Options                                                                                                                                                                                  |
|-------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| AutoHOLD<br>   | $\tilde{V}$ switch position turns on all LCD segments.<br>$\overline{\tilde{V}}$ switch position displays the software version number.<br>$m\tilde{V}$ switch position displays the model number. |
|              | Disables beeper. ( <b>bEEP</b> )                                                                                                                                                                  |
|              | Enables "Smoothing" mode. ( <b>S---</b> )<br>Dampens display fluctuations of rapidly changing inputs by digital filtering.                                                                        |
| <br>(YELLOW) | Disables automatic power-down ("Sleep mode"). ( <b>PoFF</b> )<br>Sleep mode is also disabled while the Meter is in a MIN MAX AVG Recording mode, or the AutoHOLD mode.                            |
|              | Disables automatic 2-minute backlight timeout. ( <b>LoFF</b> ) ( <b>Model 177 and 179 Only</b> )                                                                                                  |

### Making Basic Measurements


The figures on the following pages show how to make basic measurements.

When connecting the test leads to the circuit or device, connect the common (COM) test lead before connecting the live lead; when removing the test leads, remove the live lead before removing the common test lead.


#### ⚠ ⚠ Warning

To avoid electric shock, injury, or damage to the Meter, disconnect circuit power and discharge all high-voltage capacitors before testing resistance, continuity, diodes, or capacitance.

### Measuring AC and DC Voltage

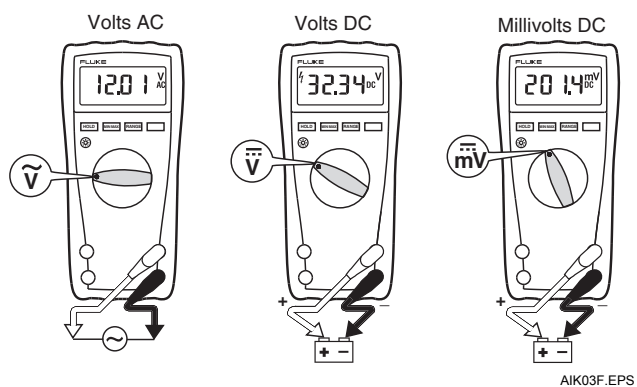


### Measuring Resistance

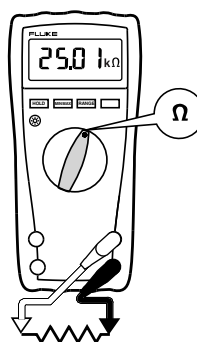


AIK04F.EPS

### Measuring Capacitance

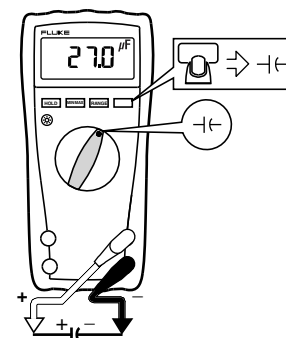


AIK05F.EPS

**Testing for Continuity**

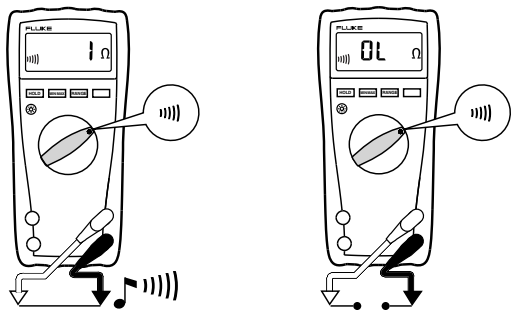

AIK06F.EPS





**Measuring Temperature (Model 179 Only)**

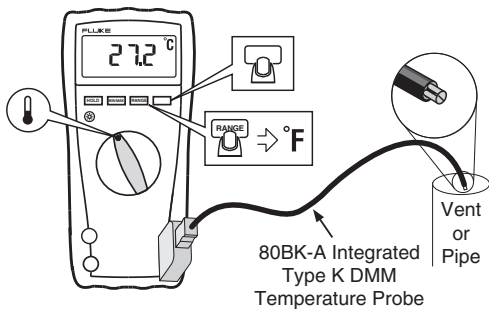

AIK10F.EPS

⚠⚠ Warning: Do not connect 80BK-A to live circuits.

**Testing Diodes**

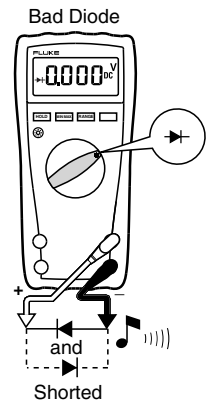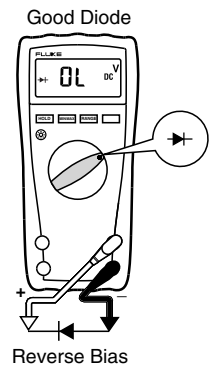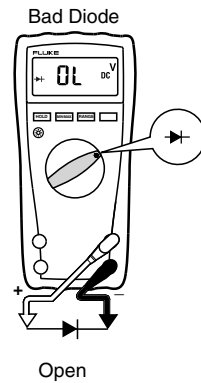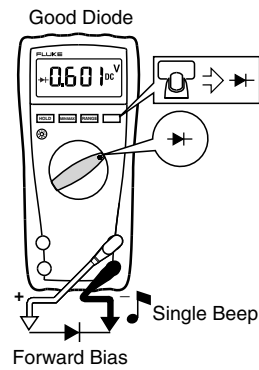

AIK07F.EPS


### Measuring AC or DC Current

#### ⚠ ⚠ Warning

To avoid personal injury or damage to the Meter:

- Never attempt to make an in-circuit current measurement when the open-circuit potential to earth is >1000 V.
- Check the Meter's fuses before testing. (See "Testing the Fuses".)
- Use the proper terminals, switch position, and range for your measurement.
- Never place the probes in parallel with a circuit or component when the leads are plugged into the current terminals.

Turn power OFF, break circuit, insert Meter in series, turn power on.

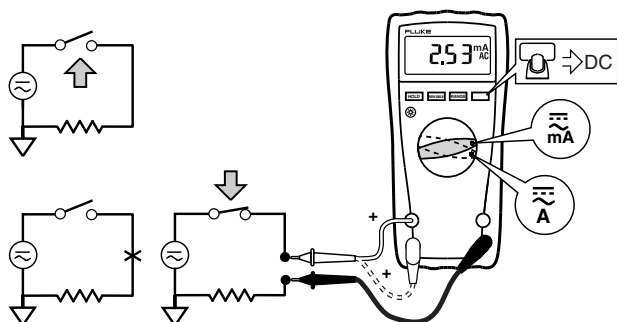

AIK08F.EPS

### Understanding AC Zero Input Behavior of True RMS Meters

Unlike averaging meters, which can accurately measure only pure sinewaves, True RMS meters accurately measure distorted waveforms. Calculating True RMS converters require a certain level of input voltage to make a measurement. This is why AC voltage and current ranges are specified from 5% of range to 100% of range. Non-zero digits that are displayed on a True RMS meter when the test leads are open or are shorted are normal. They do not affect the specified AC accuracy above 5% of range.

Unspecified input levels on the lowest ranges are:

- AC voltage: below 5% of 600 mV AC, or 30 mV AC
- AC current: below 5% of 60 mA AC, or 3 mA AC

### Measuring Frequency


#### ⚠⚠ Warning

To avoid electrical shock, disregard the bar graph for frequencies > 1 kHz. If the frequency of the measured signal is > 1 kHz, the bar graph is unspecified.

The Meter measures the frequency of a signal. The trigger level is 0 V, 0 A AC for all ranges.

AC/DC Voltage Frequency

AC Current Frequency

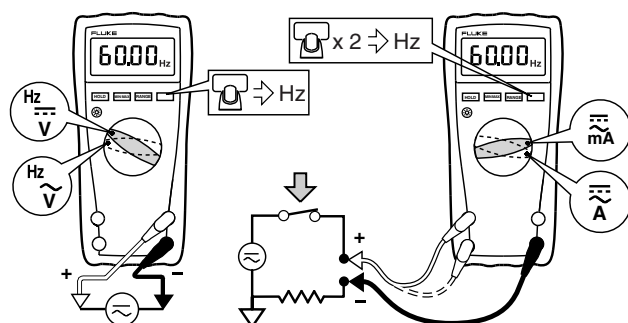

AIK09F.EPS

- ⇒ To exit frequency, press **YELLOW** button or turn the rotary switch.
- ⇒ In frequency, the bar graph shows the AC/DC voltage or AC current accurately up to 1 kHz.
- ⇒ Select progressively lower ranges using manual ranging for a stable reading.

### Using the Bar Graph

The bar graph is like the needle on an analog Meter. It has an overload indicator (▶) to the right and a polarity indicator (±) to the left.

Because the bar graph updates about 40 times per second, which is 10 times faster than the digital display, the bar graph is useful for making peak and null adjustments and for observing rapidly changing inputs.

The bar graph is disabled when measuring capacitance or temperature. In frequency, the bar graph accurately indicates the voltage or current up to 1 kHz.

The number of lit segments indicates the measured value and is relative to the full-scale value of the selected range.

In the 60 V range, for example (see below), the major divisions on the scale represent 0, 15, 30, 45, and 60 V. An input of -30 V lights the negative sign and the segments up to the middle of the scale.



AIK11F.EPS


Cleaning

Wipe the case with a damp cloth and mild detergent. Do not use abrasives or solvents. Dirt or moisture in the terminals can affect readings.

Testing the Fuses

Warning

To avoid electrical shock or injury, remove the test leads and any input signals before replacing the fuse.  
Test fuses as shown below.

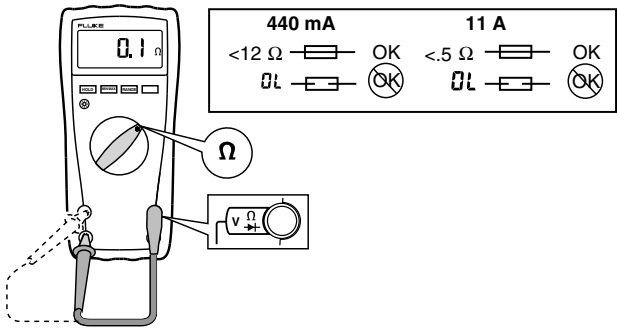


AIK12F.EPS

Replacing the Battery and Fuses

Warning

- To avoid shock, injury, or damage to the Meter:
- Use ONLY fuses with the amperage, interrupt, voltage, and speed ratings specified.
  - Replace the battery as soon as the low battery indicator ( ) appears.

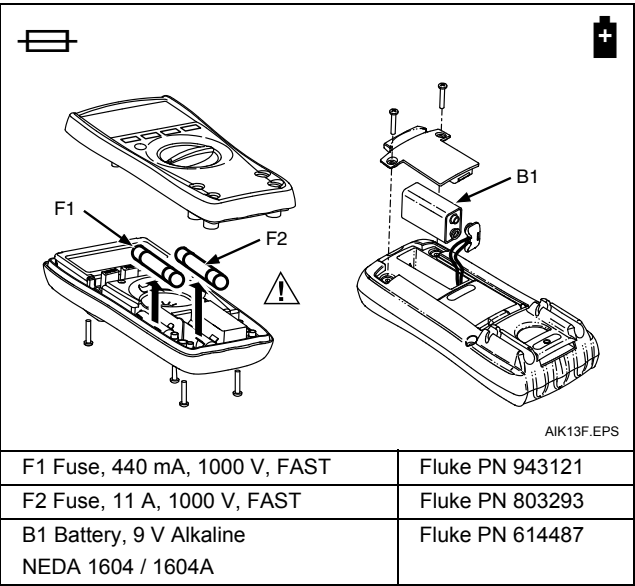

AIK13F.EPS

### Specifications

|                                                                                                                                                                                                                         |                                                                                                                                           |
|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------|
| Accuracy is specified for 1 yr after calibration, at operating temperatures of 18 °C to 28 °C, with relative humidity at 0 % to 90 %. Accuracy specifications take the form of: $\pm$ ( [ % of Reading ] + [ Counts ] ) |                                                                                                                                           |
| <b>Maximum voltage between any terminal and earth ground:</b> 1000 V DC or AC RMS                                                                                                                                       |                                                                                                                                           |
| <b>Surge Protection:</b>                                                                                                                                                                                                | 8 kV peak per IEC 61010                                                                                                                   |
| <b>⚠ Fuse for mA inputs:</b>                                                                                                                                                                                            | 440 mA, 1000 V FAST Fuse                                                                                                                  |
| <b>⚠ Fuse for A input:</b>                                                                                                                                                                                              | 11 A, 1000 V FAST Fuse                                                                                                                    |
| <b>Display:</b>                                                                                                                                                                                                         | Digital: 6000 counts, updates 4/sec<br>Bar Graph: 33 segments;<br>Updates 40/sec<br>Frequency: 10,000 counts<br>Capacitance: 1,000 counts |
| <b>Altitude:</b>                                                                                                                                                                                                        | Operating: 2000 m; Storage: 12,000 m                                                                                                      |
| <b>Temperature:</b>                                                                                                                                                                                                     | Operating: -10 °C to +50 °C;<br>Storage: -40 °C to +60 °C                                                                                 |
| <b>Temperature coefficient:</b>                                                                                                                                                                                         | 0.1 X (specified accuracy / °C<br>( < 18 °C or > 28 °C )                                                                                  |
| <b>Electromagnetic Compatibility (EN 61326-1:1997):</b>                                                                                                                                                                 | In an RF field of 3 V/M, accuracy = specified accuracy except in temperature: specified accuracy $\pm$ 5 °C (9 °F)                        |
| <b>Relative Humidity:</b>                                                                                                                                                                                               | Maximum Noncondensing<br>90 % to 35 °C<br>75 % to 40 °C<br>45 % to 50 °C                                                                  |
| <b>Battery Life:</b>                                                                                                                                                                                                    | Alkaline: 400 hrs typical                                                                                                                 |
| <b>Size (H x W x L):</b>                                                                                                                                                                                                | 4.3 cm x 9 cm x 18.5 cm                                                                                                                   |
| <b>Weight:</b>                                                                                                                                                                                                          | 420 g                                                                                                                                     |
| <b>Safety Compliances:</b>                                                                                                                                                                                              | ANSI/ISA S82.02.01, CSA C22.2-1010.1, IEC 61010 to 1000 V Measurement Category III, 600 V Measurement Category IV                         |
| <b>Certifications:</b>                                                                                                                                                                                                  | CSA, TÜV (EN61010), UL, C,  , VDE                      |

**Models 175, 177 & 179**  
Users Manual

| Function                                               | Range <sup>1</sup>        | Resolution       | Accuracy $\pm$ ( [ % of Reading ] + [ Counts ] )                                                                      |                             |                             |
|--------------------------------------------------------|---------------------------|------------------|-----------------------------------------------------------------------------------------------------------------------|-----------------------------|-----------------------------|
|                                                        |                           |                  | Model 175                                                                                                             | Model 177                   | Model 179                   |
| AC Volts <sup>2,3</sup>                                | 600.0 mV                  | 0.1 mV           | 1.0 % + 3                                                                                                             | 1.0 % + 3                   | 1.0 % + 3                   |
|                                                        | 6.000 V                   | 0.001 V          | (45 Hz to 500 Hz)                                                                                                     | (45 Hz to 500 Hz)           | (45 Hz to 500 Hz)           |
|                                                        | 60.00 V                   | 0.01 V           |                                                                                                                       |                             |                             |
|                                                        | 600.0 V                   | 0.1 V            | 2.0 % + 3 (500 Hz to 1 kHz)                                                                                           | 2.0 % + 3 (500 Hz to 1 kHz) | 2.0 % + 3 (500 Hz to 1 kHz) |
|                                                        | 1000 V                    | 1 V              |                                                                                                                       |                             |                             |
| DC mV                                                  | 600.0 mV                  | 0.1 mV           | 0.15 % + 2                                                                                                            | 0.09 % + 2                  | 0.09 % + 2                  |
| DC Volts                                               | 6.000 V                   | 0.001 V          |                                                                                                                       |                             |                             |
|                                                        | 60.00 V                   | 0.01 V           | 0.15 % + 2                                                                                                            | 0.09 % + 2                  | 0.09 % + 2                  |
|                                                        | 600.0 V                   | 0.1 V            |                                                                                                                       |                             |                             |
|                                                        | 1000 V                    | 1 V              | 0.15 % + 2                                                                                                            | 0.15 % + 2                  | 0.15 % + 2                  |
| Continuity                                             | 600 $\Omega$              | 1 $\Omega$       | Meter beeps at < 25 $\Omega$ , beeper turns off at > 250 $\Omega$ ; detects opens or shorts of 250 $\mu$ s or longer. |                             |                             |
| Ohms                                                   | 600.0 $\Omega$            | 0.1 $\Omega$     | 0.9 % + 2                                                                                                             | 0.9 % + 2                   | 0.9 % + 2                   |
|                                                        | 6.000 k $\Omega$          | 0.001 k $\Omega$ | 0.9 % + 1                                                                                                             | 0.9 % + 1                   | 0.9 % + 1                   |
|                                                        | 60.00 k $\Omega$          | 0.01 k $\Omega$  | 0.9 % + 1                                                                                                             | 0.9 % + 1                   | 0.9 % + 1                   |
|                                                        | 600.0 k $\Omega$          | 0.1 k $\Omega$   | 0.9 % + 1                                                                                                             | 0.9 % + 1                   | 0.9 % + 1                   |
|                                                        | 6.000 M $\Omega$          | 0.001 M $\Omega$ | 0.9 % + 1                                                                                                             | 0.9 % + 1                   | 0.9 % + 1                   |
|                                                        | 50.00 M $\Omega$          | 0.01 M $\Omega$  | 1.5 % + 3                                                                                                             | 1.5 % + 3                   | 1.5 % + 3                   |
| Diode test                                             | 2.400 V                   | 0.001 V          | 1 % + 2                                                                                                               |                             |                             |
| Capacitance                                            | 1000 nF                   | 1 nF             | 1.2 % + 2                                                                                                             | 1.2 % + 2                   | 1.2 % + 2                   |
|                                                        | 10.00 $\mu$ F             | 0.01 $\mu$ F     | 1.2 % + 2                                                                                                             | 1.2 % + 2                   | 1.2 % + 2                   |
|                                                        | 100.0 $\mu$ F             | 0.1 $\mu$ F      | 1.2 % + 2                                                                                                             | 1.2 % + 2                   | 1.2 % + 2                   |
|                                                        | 9999 $\mu$ F <sup>4</sup> | 1 $\mu$ F        | 10 % typical                                                                                                          | 10 % typical                | 10 % typical                |
| AC Amps <sup>5</sup><br>(True RMS)<br>(45 Hz to 1 kHz) | 60.00 mA                  | 0.01 mA          |                                                                                                                       |                             |                             |
|                                                        | 400.0 mA <sup>6</sup>     | 0.1 mA           | 1.5 % + 3                                                                                                             | 1.5 % + 3                   | 1.5 % + 3                   |
|                                                        | 6.000 A                   | 0.001 A          |                                                                                                                       |                             |                             |
|                                                        | 10.00 A <sup>7</sup>      | 0.01 A           |                                                                                                                       |                             |                             |

1. All AC voltage and AC current ranges are specified from 5 % of range to 100 % of range.
2. Crest factor of  $\leq 3$  at full scale up to 500 V, decreasing linearly to crest factor  $\leq 1.5$  at 1000 V.
3. For non-sinusoidal waveforms, add -(2% reading + 2% full scale) typical, for crest factors up to 3.
4. In the 9999  $\mu$ F range for measurements to 1000  $\mu$ F, the measurement accuracy is 1.2 % + 2 for all models.
5. Amps input burden voltage (typical): 400 mA input 2 mV/mA, 10 A input 37 mV/A.
6. 400.0 mA accuracy specified up to 600 mA overload.
7. > 10A unspecified.

**True RMS Multimeters**  
Specifications

| Function                                                                                                                                                                                                                                                                                                                                                                                                                                                            | Range <sup>1</sup>                                                                                                                                                                                                                                                                 | Resolution                                 | Accuracy ±( [ % of Reading ] + [ Counts ] ) |           |                                                |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------|---------------------------------------------|-----------|------------------------------------------------|
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |                                                                                                                                                                                                                                                                                    |                                            | Model 175                                   | Model 177 | Model 179                                      |
| DC Amps <sup>4</sup>                                                                                                                                                                                                                                                                                                                                                                                                                                                | 60.00 mA<br>400.0 mA <sup>6</sup><br>6.000 A<br>10.00 A <sup>7</sup>                                                                                                                                                                                                               | 0.01 mA<br>0.1 mA<br>0.001 A<br>0.01 A     | 1.0 % + 3                                   | 1.0 % + 3 | 1.0 % + 3                                      |
| Hz<br>(AC- or DC-<br>coupled, V or<br>A <sup>2,3</sup> input )                                                                                                                                                                                                                                                                                                                                                                                                      | 99.99 Hz<br>999.9 Hz<br>9.999 kHz<br>99.99 kHz                                                                                                                                                                                                                                     | 0.01 Hz<br>0.1 Hz<br>0.001 kHz<br>0.01 kHz | 0.1 % + 1                                   | 0.1 % + 1 | 0.1 % + 1                                      |
| Temperature                                                                                                                                                                                                                                                                                                                                                                                                                                                         | -40 °C to +400 °C<br>-40 °F to +752 °F                                                                                                                                                                                                                                             | 0.1 °C<br>0.1 °F                           | NA                                          | NA        | 1 % + 10 <sup>5</sup><br>1 % + 18 <sup>5</sup> |
| MIN MAX AVG                                                                                                                                                                                                                                                                                                                                                                                                                                                         | For DC functions, accuracy is the specified accuracy of the measurement function ±12 counts for changes longer than 350 ms in duration.<br>For AC functions, accuracy is the specified accuracy of the measurement function ±40 counts for changes longer than 900 ms in duration. |                                            |                                             |           |                                                |
| 1. All AC voltage and AC current ranges are specified from 5 % of range to 100 % of range.<br>2. Frequency is specified from 2 Hz to 99.99 kHz in Volts and from 2 Hz to 30 kHz in Amps.<br>3. Below 2 Hz, the display shows zero Hz.<br>4. Amps input burden voltage (typical): 400 mA input 2 mV/A, 10 A input 37 mV/A.<br>5. Does not include error of the thermocouple probe.<br>6. 400.0 mA accuracy specified up to 600 mA overload.<br>7. > 10A unspecified. |                                                                                                                                                                                                                                                                                    |                                            |                                             |           |                                                |

**Models 175, 177 & 179**  
Users Manual

| Function                                                               | Overload Protection <sup>1</sup> | Input Impedance (Nominal)         | Common Mode Rejection Ratio (1 kΩ Unbalanced)               |                                                                | Normal Mode Rejection    |
|------------------------------------------------------------------------|----------------------------------|-----------------------------------|-------------------------------------------------------------|----------------------------------------------------------------|--------------------------|
| Volts AC                                                               | 1000 V RMS                       | > 10 MΩ < 100 pF                  | > 60 dB @ DC, 50 Hz or 60 Hz                                |                                                                |                          |
| Volts DC                                                               | 1000 V RMS                       | > 10 MΩ < 100 pF                  | >120 dB @ DC, 50 Hz or 60 Hz                                |                                                                | > 60 dB @ 50 Hz or 60 Hz |
| mV/μ                                                                   | 1000 V RMS <sup>2</sup>          | > 10 MΩ < 100 pF                  | >120 dB @ DC, 50 Hz or 60 Hz                                |                                                                | > 60 dB @ 50 Hz or 60 Hz |
|                                                                        |                                  | Open Circuit Test Voltage         | Full Scale Voltage To:<br>600 kΩ                      50 MΩ |                                                                | Short Circuit Current    |
| Ohms/Capacitance                                                       | 1000 V RMS <sup>2</sup>          | < 8.0 V DC                        | < 660 mV DC                                                 | < 4.6 V DC                                                     | < 1.1 mA                 |
| Continuity/Diode test                                                  | 1000 V RMS <sup>2</sup>          | < 8.0 V DC                        | 2.4 V DC                                                    |                                                                | < 1.1 mA                 |
| 1. 10 <sup>7</sup> V-Hz maximum.                                       |                                  |                                   |                                                             |                                                                |                          |
| 2. For circuits < 0.3 A short circuit. 660 V for high energy circuits. |                                  |                                   |                                                             |                                                                |                          |
| Function                                                               |                                  | Overload Protection               |                                                             | Overload                                                       |                          |
| mA                                                                     |                                  | Fused, 44/100 A, 1000 V FAST Fuse |                                                             | 600 mA overload for 2 minutes maximum, 10 minutes rest minimum |                          |
| A                                                                      |                                  | Fused, 11 A, 1000 V FAST Fuse     |                                                             | 20 A overload for 30 seconds maximum, 10 minutes rest minimum  |                          |